

Dorothea Hansen, Daniel Benner, Martin Hilgenhaener, Therese Leisebein, Andreas Brauksiepe, Walter Popp Krankenhaushygiene, Universitaetsklinikum Essen, Germany

German Medical Science 2004;2:Doc04

### **Abstracts**

Insufficient performance of cleaning and disinfection of flexible endoscopes can pose an infection risk to patients. Actually quality of reprocessing is checked by performing microbiological cultures. Unfortunately, their results are not available on the same day so that more rapid methods are desirable. We compared the ATP (adenosine triphosphate) bioluminescence for hygiene checking of the reprocessing procedures of 108 flexible endoscopes with routine microbiological culture technics.

Sensitivity and specificity of ATP bioluminescence was calculated. 28 endoscopes showed bacterial growth of at least one sample. Depending on the applied threshold of bioluminescence between 67 and 28 endoscopes were positive. Sensitivity varied between 0.46 and 0.75 and specificity between 0.43 and 0.81. ATP bioluminescence does not replace routine microbiologic methods but it can indicate the need of immediate check of reprocessing.

### **Introduction**

Infections by endoscopes have been described as a consequence of insufficient cleaning and disinfection [1], [2]. Reports regard duodenoscopes [3], coloscopes [4], and bronchoscopes [5], [6] and concern exists regarding the possible transmission of infective agents like hepatitis B-/C- virus, HIV, Mycobacterium tuberculosis and Helicobacter pylori [7]. An investigation in southern Germany has shown that 50% of endoscopes were still contaminated by bacteria after reprocessing [8] American [9], [10], [11] and European [7], [12], [13], [14], [15] recommendations for their processing of endoscopes have been published. Whereas in Germany and various other countries control of cleaning and disinfection by microbiological methods is recommended the use of microbiological cultures to routinely check the reprocessing process is discussed controversially in USA [7], [16]. Unfortunately, there are many disadvantages of microbiological cultures: Getting results lasts for days, so the endoscopes are used with other patients. Additionally, viruses, Helicobacter and M. tuberculosis are not at all included and slowly growing organisms only if the time of incubation is long enough. So a more rapid method for checking the reprocessing of endoscopes is needed. ATP (adenosine triphosphate) measurement is used as indicator of cleaning control [17], [18] in food and kitchen hygiene. ATP is as well an indicator of organic as of microbiological contamination. It is a simple method measuring the amount of light which is emitted when the enzyme luciferase comes into contact with molecular ATP and which is directly proportional to the amount of ATP [19]. ATP measurement may be a suitable method to control the quality of endoscope reprocessing as it is measuring cleaning effectiveness which may indicate the reduction of infection risk.

We did an investigation to compare the ATP bioluminescence for hygiene checking of reprocessing with routine microbiological cultures.

## Methods

Between January and December 2003 we examined 108 endoscopes (40 gastroscopes, 18 coloscopes, 8 duodenoscopes and 42 bronchoscopes) after reprocessing. Sterile swabs were moistened with sterile 0.9% NaCl. We took swabs of distal end and rinsing valve and rinsed the operating channel with 20 ml sterile 0.9% NaCl. We did not use neutralizers. Swabs and 0.5 ml of rinsing fluid were inoculated on blood agar, MacConkey agar and Sabouraud agar and incubated for 48 hours at 37° C and 7 days at 22° C respectively. Bacterial species identification followed routine microbial laboratory proceedings (API biomérieux). Every bacterial growth was considered microbiological positive regardless of species or number of cfu (colony forming unit). ATP and AMP (adenosine monophosphate) bioluminescence was determined using Lumitester PD 10 (Scil Diagnostics). The assay was carried out according to the manufacturer's instructions immediately after swabbing.

Reagent blanks were obtained using sterile swabs moistened with sterile 0.9% NaCl, instrument disinfectant and endoscope cleaner used for endoscope reprocessing. Bioluminescence readings were expressed as relative light units (RLU). Thresholds for bioluminescence were chosen between 30 and 100 RLU according to manufacturer's personal recommendation and after determining RLU of disinfectant and cleaner below 10 RLU. Sensitivity and specificity of ATP bioluminescence compared with microbiological culture as a gold standard were calculated for all types of examined endoscopes together and displayed in a ROC curve for various threshold values. The area under the ROC curve, which is usually chosen as the summary measure of diagnostic accuracy, was also computed.

## Results

Results of microbiological culture and ATP bioluminescence are shown in Table 1. Microbiological cultures of 28 endoscopes (26%) showed bacterial growth. 13% of checked duodenoscopes, 28% of coloscopes, 23% of gastroscopes and 31% of bronchoscopes were bacterially contaminated. The detected organisms were *Pseudomonas aeruginosa*, other non fermenting gramnegative rods, Enterobacteriaceae, *Staphylococcus aureus*, koagulase negative *Staphylococci*, *Corynebacteriae*, Bacilli, *Candida* and moulds. Dependent on the chosen threshold between 28 (26%) and 67 (62%) Hansen et al. ATP measurement as method to monitor the quality of reprocessing flexible endoscopes.

Endoscopes were positive for ATP bioluminescence. ATP bioluminescence of 75% of duodenoscopes, 67% of coloscopes, 63% of gastroscopes and 57% of bronchoscopes was above a threshold of 30 RLU. There were still 25% of duodenoscopes, 50% of coloscopes, 30% of gastroscopes and 24% of bronchoscopes above a threshold of 100 RLU. ATP bioluminescence of 5 bronchoscopes and 2 gastroscopes was below 30 RLU despite being microbiologically contaminated. Choosing 30 RLU as threshold 21 endoscopes (8 bronchoscopes, 7 gastroscopes, 5 coloscopes and 1 duodenoscope) were positive for ATP bioluminescence and microbiological culture and 34 endoscopes (13 bronchoscopes, 13 gastroscopes, 6 coloscopes and 2 duodenoscopes) were negative. 46 endoscopes (16 bronchoscopes, 18 gastroscopes, 7 coloscopes and 5 duodenoscopes) had an ATP bioluminescence above 30 RLU despite negative microbiological result. Above a threshold of 100 RLU 65 endoscopes (24 bronchoscopes, 23 gastroscopes, 12 coloscopes and 6 duodenoscopes) had concordant negative and 13 endoscopes (5 bronchoscopes, 4 gastroscopes, 3 coloscopes and 1 duodenoscope) concordant positive results. Microbiological cultures of 15 endoscopes (5 bronchoscopes, 8 gastroscopes, 1 coloscope and 1 duodenoscope) were negative despite ATP bioluminescence above 100 RLU. The ROC curve of sensitivity and specificity for thresholds between

30 and 100 RLU is presented in Figure 1. The area under the ROC curve is 0.63. Compared with microbiological culture as a gold standard sensitivity of bioluminescence varied between 0.75 for a threshold of 30 RLU (95% confidence interval 0.55-0.89) and 0.46 for 100 RLU (95% confidence interval 0.28-0.66) and specificity between 0.43 (95% confidence interval 0.32-0.54) and 0.81 (95% confidence interval 0.71-0.89) respectively (Tab. 2).

## **Discussion**

In our study, 26% of tested endoscopes showed microbiological contamination. The number of contaminated endoscopes in our investigation is in accordance with the results of Moses and Lee [20], who found between 12% and 24% positive cultures during a 10-year study period. It is much lower than that of the HYGEA study [8]. Moses and Lee examined only endoscopes used in a clinical institution and reprocessed in an automated washer whereas in half of endoscopy facilities of the HYGEA study endoscopes were reprocessed manually. In our study 92 endoscopes (85%) were reprocessed in an automated washer. 3 Dependent on the chosen threshold between 62% and 26% of the tested endoscopes had a positive bioluminescence result indicating possible organic contamination. In order to calculate sensitivity and specificity of ATP bioluminescence there must be another method which truly indicates contamination of reprocessed endoscopes. The only established method for checking endoscope reprocessing is microbiological culture. Microbiological culture may fail in indicating all contaminated endoscopes. There may be non viable organisms or organisms which cannot be cultured on conventional culture medium and other than bacterial contaminations are possible.

Because of the absence of other methods for checking endoscopes we calculated sensitivity and specificity of ATP bioluminescence compared to microbiological culture as gold standard. Sensitivity and specificity of bioluminescence differ dependent on the chosen threshold. In our study sensitivity was only 0.75 even when the chosen threshold of RLU was low. The ROC curve of ATP bioluminescence presented in Figure 1 with an area under the curve of 0.63 indicates that there is no strong concordance between ATP bioluminescence and microbiological culture. Our results are similar to those found by Murphy et al. [18] for testing food contact surfaces. Murphy et al. suspected that conventional microbiology is more sensitive than ATP bioluminescence when total ATP is low [18]. Bacterial ATP content may be below the limit of ATP bioluminescence. Different bacterial specimen can contain different amounts of ATP and the amount of ATP also depends on the metabolism of the organisms [19]. ATP bioluminescence may also be influenced by the number of viable bacteria present. We did not differ between kind of specimen and number of cfu cultured. The number of cfu found on most swabs was very low and this may explain the low sensitivity of ATP bioluminescence compared to routine microbiology in our study. Additionally the low specificity of ATP bioluminescence may be explained by the fact, that not only viable bacteria but also other organic contamination is detected. Similar to our study Poulis et al. [21] could not find a clear relationship between ATP bioluminescence measurements and number of cfu on surface plates under practical conditions on surfaces in a factory. Alfa et al. [22] reported that the presence of high residual soil (protein, carbohydrate, hemoglobin and endotoxin) did not correlate with microbiological contamination of reprocessed endoscopes. Thus measurable ATP bioluminescence may indicate contamination of endoscopes without presence of cultivable microorganisms. Reprocessed endoscopes should be clean. A clean endoscope should not only show a less amount of viable organisms but also a less amount of all organic contamination and ATP sources. The presence of any ATP source may indicate an infectious risk for consecutively examined patients and should be avoided irrespective of cultivable bacteria.

We conclude that ATP bioluminescence does not replace routine microbiologic methods but it should be applied additionally to check endoscope reprocessing. In contrast to microbiologic methods results of ATP bioluminescence are available at once and can indicate the need for checking the reprocessing practice immediately.

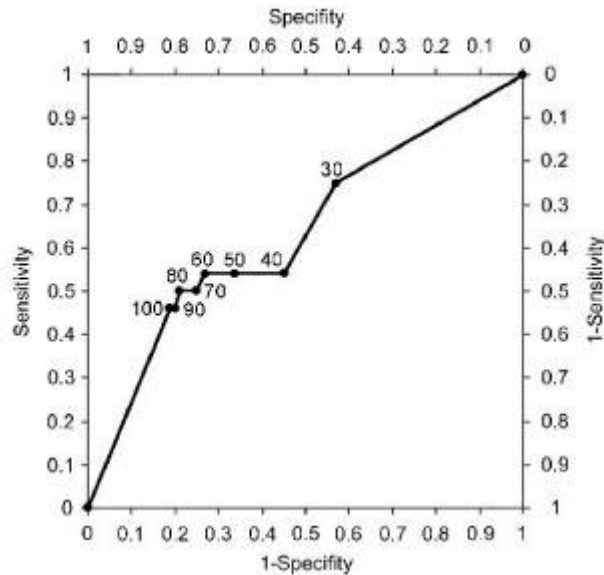


Figure 1: ROC curve of bioluminescence compared with microbiological culture as gold standard for thresholds between 30 and 100 RLU

Kind of endoscope	Microbiological culture	Threshold (RLU)							
		>30	>40	>50	>60	>70	>80	>90	>100
bronchoscope n=42	positive n=13	8	5	5	5	5	5	5	5
	negative n=29	16	15	8	6	5	5	5	5
gastroscope n=40	positive n=9	7	5	5	5	5	5	4	4
	negative n=31	18	14	12	10	9	8	8	8
coloscope n=18	positive n=5	5	4	4	4	3	3	3	3
	negative n=13	7	4	4	3	3	2	2	1
duodenoscope n=8	positive n=1	1	1	1	1	1	1	1	1
	negative n=7	5	3	3	3	3	2	1	1
all endoscopes n=108	positive n=28	21	15	15	15	14	14	13	13
	negative n=80	46	36	27	22	20	17	16	15

Table 1: Number of endoscopes with a bioluminescence value above the threshold compared with microbiological culture Threshold (RLU) Sensitivity.

Threshold (RLU)	Sensitivity (95% confidence interval)	Specificity (95% confidence interval)
30	0.75 (0.55-0.89)	0.43 (0.32-0.54)
40	0.54 (0.34-0.72)	0.55 (0.47-0.66)
50	0.54 (0.34-0.72)	0.66 (0.54-0.76)
60	0.54 (0.34-0.72)	0.73 (0.61-0.82)
70	0.50 (0.31-0.69)	0.75 (0.64-0.84)
80	0.50 (0.31-0.69)	0.79 (0.68-0.87)
90	0.46 (0.28-0.66)	0.80 (0.70-0.88)
100	0.46 (0.28-0.66)	0.81 (0.71-0.89)

Table 2: Sensitivity and specificity of bioluminescence as compared with microbiological culture and 95% confidence interval

## References

1. Nelson DB, Barkun AN, Block KP, Burdick JS, Ginsberg GG, Greenwald DA, Kelsey PB, Nakao NL, Slivka A, Smith P, Vakil N. Technology status evaluation report. Transmission of infection by gastrointestinal endoscopy. May 2001. *Gastrointest Endosc.* 2001;54(6):824-8.
2. Cowen AE. The clinical risks of infection associated with endoscopy. *Can Gastroenterol.* 2001;15(5):321-31.
3. Langenberg W, Rauws EA, Oudbier JH, Tytgat GN. Patient-to-patient transmission of *Campylobacter pylori* infection by fiberoptic gastroduodenoscopy and biopsy. *J Infect Dis.* 1990;161(3):507-11.
4. Bronowicki JP, Venard V, Botte C, Monhoven N, Gastin I, Chone L, Hudziak H, Rihn B, Delanoe C, LeFaou A, Bigard MA, Gaucher P. Patient-to-patient transmission of hepatitis C virus during colonoscopy. *N Engl J Med.* 1997;337(4):237-40.
5. Bronchoscopy-related infections and pseudoinfections--New York, 1996 and 1998. *MMWR Morb Mortal Wkly Rep.* 1999;48(26):557-60.
6. Ramsey AH, Oemig TV, Davis JP, Massey JP, Torok TJ. An outbreak of bronchoscopy-related *Mycobacterium tuberculosis* infections due to lack of bronchoscope leak testing. *Chest.* 2002;121(3):976-81.
7. Anforderungen an die Hygiene bei der Aufbereitung flexibler Endoskope und endoskopischen Zusatzinstrumentariums. Empfehlung der Kommission f1 D4r Krankenhaushygiene und Infektionsprvention beim Robert Koch-Institut (RKI). *Bundesgesundheitsbl Gesundheitsforsch Gesundheitsschutz.* 2002;45(4):395-411.
8. Bader L, Blumenstock G, Birkner B, Leiss O, Heesemann J, Riemann JF, Selbmann HK. HYGEA (Hygiene in der Gastroenterologie - Endoskop-Aufbereitung): Studie zur Qualitt der Aufbereitung von flexiblen Endoskopen in Klinik und Praxis. *Z Gastroenterol.* 2002;40(3):157-70.
9. Nelson DB, Jarvis WR, Rutala WA, Foxx-Orenstein AE, Isenberg G, Dash GR, Alvarado CJ, Ball M, Griffin-Sobel J, Petersen C, Ball KA, Henderson J, Stricof RL; Society for Healthcare Epidemiology of America. Multi-society guideline for reprocessing flexible gastrointestinal endoscopes. Society for Healthcare Epidemiology of America. *Infect Control Hosp Epidemiol.* 2003;24(7):532-7.
10. Reprocessing of flexible gastrointestinal endoscopes. *American Society for Gastrointestinal Endoscopy. Gastrointest Endosc.* 1996;43(5):540-5.
11. Alvarado CJ, Reichelderfer M. APIC guideline for infection prevention and control in flexible endoscopy. Association for Professionals in Infection Control. *Am J Infect Control.* 2000;28(2):138-55.
12. Cleaning and disinfection of equipment for gastrointestinal endoscopy. Report of a Working Party of the British Society of Gastroenterology Endoscopy Committee. *Gut.* 1998;42(4):585-93.
13. Systchenko R, Marchetti B, Canard JN, Palazzo L, Ponchon T, Rey JF, Sautereau D; French Society of Digestive Endoscopy. Guidelines of the French Society of Digestive Endoscopy: recommendations for setting up cleaning and disinfection procedures in gastrointestinal endoscopy. *Endoscopy.* 2000;32(10):807-18.
14. Bundesrztekammer. Empfehlung zur Qualittssicherung in der gastrointestinalen Endoskopie. *Dtsch rztebl.* 2000;97(8):A475-A477.
15. Anforderungen der Hygiene an die baulich-funktionelle Gestaltung und apparative Ausstattung von Endoskopieeinheiten. Empfehlung der Kommission f1 D4r Krankenhaushygiene und Infektionsprvention beim Robert Koch-Institut. *Bundesgesundheitsbl Gesundheitsforsch*

Gesundheitsschutz. 2002;45(4):412-4.

16. Leung J, Vallerio R, Wilson R. Surveillance cultures to monitor quality of gastrointestinal endoscope reprocessing. *Am J Gastroenterol.* 2003;98(1):3-5.
17. Seeger K, Griffiths MW. Adenosine triphosphate bioluminescence for hygiene monitoring in health care institutions. *J Food Prot.* 1994;57(6):509-12.
18. Murphy SC, Kozlowski SM, Bandler DK, Boor KJ. Evaluation of adenosine triphosphate-bioluminescence hygiene monitoring for trouble-shooting fluid milk shelf-life problems. *J Dairy Sci.* 1998;81(3):817-20.
19. Baumgart J. Möglichkeiten und Grenzen moderner Schnellverfahren zur Prozesskontrolle von Reinigungs- und Desinfektionsverfahren. *Zentralbl Hyg Umweltmed.* 1996;199(2-4):366-75.
20. Moses FM, Lee J. Surveillance cultures to monitor quality of gastrointestinal endoscope reprocessing. *Am J Gastroenterol.* 2003;98(1):77-81.
21. Poulis JA, de Pijper M, Mossel DA, Dekkers PP. Assessment of cleaning and disinfection in the food industry with the rapid ATP-bioluminescence technique combined with the tissue fluid contamination test and a conventional microbiological method. *Int J Food Microbiol.* 1993;20(2):109-16.
22. Alfa MJ, Olson N, DeGagne P, Jackson M. A survey of reprocessing methods, residual viable bioburden, and soil levels in patient-ready endoscopic retrograde cholangiopancreatography duodenoscopes used in Canadian centers. *Infect Control Hosp Epidemiol.* 2002;23(4):198-206.