


N-Glycan Array User Manual

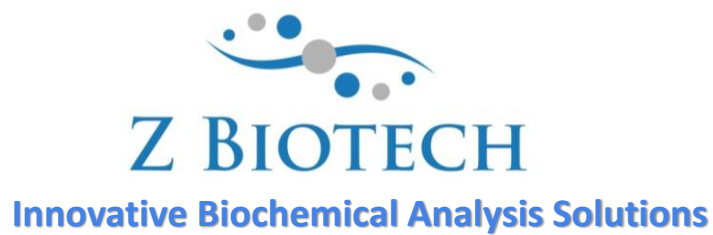

Website: <http://www.zbiotech.com/home.html>

Tel: (720) 285-3587

Email: info@zbiotech.com

For Research Use Only

Copyright 2021, Z Biotech, LLC. All Rights Reserved.

Introduction

Glycans attached to cell membranes and other types of proteins are the primary determinants for binding activity and consecutive cellular function. The study of the function and characteristics of these sugars is a fundamental part of immunology research and is applicable in understanding a variety of intercellular interactions. New technologies such as microarrays for glycan-binding applications allow researchers to investigate and reveal new information about this wide and developing field of glycoscience.

Z Biotech's N-Glycan Array is used as a general test to help researchers determine binding characteristics of antibodies, proteins, bacteria, cell cultures, or other potential biological samples to an array of 100 fundamental N-glycans. Our microarray slides are especially coated to be capable of immobilizing natural N-glycans with close-ring structure at their reducing end (GlcNAc). N-linked oligosaccharides in particular play a major role in intercellular interactions and immune cell functions, making them often preferred glycan candidates for the study of carbohydrate-binding-vaccines, such as HIV Broadly Neutralizing Antibodies. The fundamental N-glycan structures provided in this array can provide understanding of basal binding determinants for antibodies or other proteins of interest. This manual is provided as a comprehensive guide to help the researcher acquire clear results from the assay. Please read through carefully before starting your experiment.


Handling and Storage

Store the bag of slides and any buffers in a 4°C refrigerator if they are to be assayed within 24 hours upon receipt. For long term storage keep the bag of slides at -20°C. Avoid freezing and thawing multiple times. Purchased slides and buffers should be used within 6 months.

Allow the bag of slides to equilibrate to room temperature at least 20 minutes before opening. After opening, re-seal any unused slides in the moisture barrier bag with a desiccant inside and refreeze.

Array Map/Schematic

N-Glycan Array slides have either 8 or 16 subarrays. Arrays are printed on the side with the "Z Biotech" label and 4-digit number ID facing upward. The "Z Biotech" label is located on the bottom center from a landscape view. The number ID is consistent with the barcode ID on the bottom from a portrait view. Dimensions and array maps are shown below.

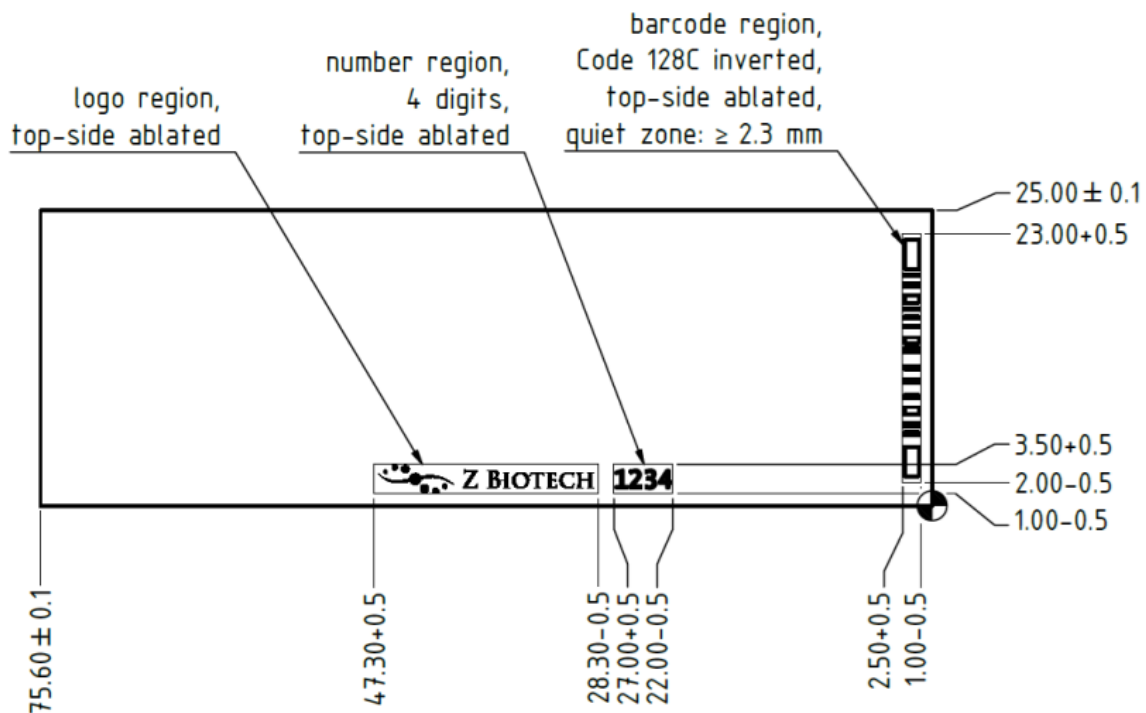

59	N223	Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-6(Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
60	N224	Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-6(Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
61	N225	Neu5Acα2-3Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-6(Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
62	N233	Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-6(Neu5Acα2-3Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
63	N234	Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-6(Neu5Acα2-3Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
64	N244	Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-6(Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
65	N255	Neu5Acα2-3Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-6(Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
66	N6000	GlcNAcβ1-2Manα1-6(GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
67	N6030	Manα1-6(GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
68	N6111	GlcNAcβ1-2Manα1-6(Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
69	N6112	GlcNAcβ1-2Manα1-6(Neu5Acα2-3Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
70	N6113	GlcNAcβ1-2Manα1-6(Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
71	N6122	Galβ1-4GlcNAcβ1-2Manα1-6(Neu5Acα2-3Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
72	N6123	Galβ1-4GlcNAcβ1-2Manα1-6(Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
73	N6144	Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-6(Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
74	N6211	Galβ1-4GlcNAcβ1-2Manα1-6(GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
75	N6212	Neu5Acα2-3Galβ1-4GlcNAcβ1-2Manα1-6(GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
76	N6213	Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-6(GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
77	N6222	Neu5Acα2-3Galβ1-4GlcNAcβ1-2Manα1-6(Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
78	N6223	Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-6(Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
79	N6244	Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-6(Neu5Acα2-6Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4(Fuca1-6)GlcNAc-
80	N3001	Galβ1-4GlcNAcβ1-2Manα1-6(Galβ1-4GlcNAcβ1-2(Galβ1-4GlcNAcβ1-4)Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
81	N3004	Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-6(Galβ1-4(Fuca1-3)GlcNAcβ1-2(Galβ1-4(Fuca1-3)GlcNAcβ1-4)Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
82	Man-1	Manβ1-4GlcNAcβ1-4GlcNAc-
83	Man-2A	Manα1-6Manβ1-4GlcNAcβ1-4GlcNAc-
84	Man-2B	Manα1-3Manβ1-4GlcNAcβ1-4GlcNAc-
85	Man-3	Manα1-6(Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
86	Man-5	Manα1-6(Manα1-3)Manα1-6(Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
87	Man-6	Manα1-6(Manα1-3)Manα1-6(Manα1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
88	Man-6D2	Manα1-6(Manα1-2Manα1-3)Manα1-6(Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
89	Man-7	[Manα1-2]Manα1-6(Manα1-3)Manα1-6(Manα1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc- (3 isomers)
90	Man-8	[Manα1-2] [Manα1-2] Manα1-6(Manα1-3)Manα1-6(Manα1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc- (3 isomers)
91	Man-9	Manα1-2Manα1-6(Manα1-2Manα1-3)Manα1-6(Manα1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
92	N002G	Neu5Gca2-3Galβ1-4GlcNAcβ1-2Manα1-6(Neu5Gca2-3Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
93	N003G	Neu5Gca2-6Galβ1-4GlcNAcβ1-2Manα1-6(Neu5Gca2-6Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
94	N012G	Manα1-6(Manα1-3)Manα1-6(Neu5Gca2-3Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
95	N013G	Manα1-6(Manα1-3)Manα1-6(Neu5Gca2-6Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
96	N015G	Manα1-6(Manα1-3)Manα1-6(Neu5Gca2-3Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
97	N022G	Neu5Gca2-3Galβ1-4GlcNAcβ1-2Manα1-3Manβ1-4GlcNAcβ1-4GlcNAc-
98	N025G	Neu5Gca2-3Galβ1-4(Fuca1-3)GlcNAcβ1-2Manα1-3Manβ1-4GlcNAcβ1-4GlcNAc-
99	N112G	GlcNAcβ1-2Manα1-6(Neu5Gca2-3Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-
100	N113G	GlcNAcβ1-2Manα1-6(Neu5Gca2-6Galβ1-4GlcNAcβ1-2Manα1-3)Manβ1-4GlcNAcβ1-4GlcNAc-

Controls

NC: Negative control; print buffer

PC1: Positive control 1; biotinylated mannose (0.01 mg/ml)

PC2: Positive control 2; human IgG (0.1 mg/ml)

PC3: Positive control 3; mouse IgG (0.1 mg/ml)

PC4: Positive control 4; rabbit IgG (0.1 mg/ml)

Array Marker: Streptavidin-Cy3 (0.01 mg/ml) + Streptavidin-Cy5 (0.01 mg/ml)

Materials Required

- Arrayed glass slides
- 16 or 8 cassettes
- Glycan Array Blocking Buffer (GABB, Item #10106), add 1% BSA (10 mg/ml) if needed
- Glycan Array Assay Buffer (GAAB, Item #10107), add 1% BSA (10 mg/ml) if needed
- Wash Buffer: 50 mM Tris-HCl, 137 mM NaCl, 0.05% Tween 20, pH 7.6

- Laser fluorescence scanner (able to scan at the wavelength of your fluorophore)
- Coplin jar
- Adhesive slide cover film

Preparation of assay samples:

Prepare glycan-binding protein samples or secondary antibodies of interest in a centrifuge tube by diluting with the Glycan Array Assay Buffer. We recommend a range of 50 µg/ml to 0.1 µg/ml concentration for protein samples, although some experimentation may be required to establish the concentration that will provide the highest binding signals with the lowest background fluorescence. This can be accomplished by applying a different dilution of samples to different wells of the array. We also suggest setting up control assays to test detection antibodies or proteins alone in case they have non-specific binding to glycans. For the fluorescently labelled streptavidin we recommend a concentration of 1 µg/mL. Calculate the volume of sample needed depending on how many slides and subarrays are to be assayed. Use 100 µL volume of sample per well for 16 subarray cassettes and 200 µL for 8 subarray cassettes in order to ensure full and even coverage of the printed area throughout incubation. If necessary, the assay can be done successfully with a minimal volume of 60 µL per well for 16 subarray cassettes and 80 µL for 8 subarrays. Using a minimal volume in the wells has an increased risk of the array drying out during the assay, and may also cause unequal distribution of the sample across the arrayed surface which may result in signal variation. Please ensure each sample is homogeneous and thoroughly mixed.

Assay Protocol

Part 1 – Blocking

Handle the slide in a clean, dry environment. Use gloves and avoid touching the slide surface.

1. Allow the arrayed slides to equilibrate to room temperature (20-30 minutes) before opening the moisture barrier bag. If the slide was ordered with the Microarray Starter Kit it will already have a cassette mounted onto it. If not, affix a cassette to the slide.
2. Add blocking buffer to each subarray well. We recommend using 100 µL per well for 16 subarray cassettes and 200 µL for 8 subarray cassettes in order to ensure full and even coverage of the printed area throughout incubation.
3. Cover the wells with adhesive film to prevent evaporation and incubate slide on shaker at 85 rpm for 1 hour. Longer incubation time is acceptable, but not necessary.

Make sure the orbital shaker is completely flat. If the slide is sloped in any direction during incubation it can cause variation in binding and detection.

Part 2 – Binding assay

1. Unless the glycan binding protein sample of interest is bacteria or cells, centrifuge samples briefly to avoid adding irrelevant particles to the array.
2. Touch the pipette tip to the corner of the well of the cassette and tip the slide so that the sample pools to that corner and remove the blocking buffer. Avoid touching the array surface.
3. Immediately apply the glycan binding protein sample of interest to each well. We recommend using 100 µL per well for 16 subarray cassettes and 200 µL for 8 subarray cassettes in order to ensure full and even coverage of the printed area throughout incubation. Avoid leaving air bubbles.
4. Seal the wells with adhesive film to prevent evaporation. If the sample is fluorescently labelled, cover with aluminum foil to keep it in the dark. Incubate on the shaker for 1-3 hours at 100 rpm. If the samples can easily aggregate, shake at higher speed to prevent protein aggregation. Longer incubation time may increase binding signal, especially for weakly binding samples.

Avoid allowing the slides to dry out at any point during the assay, especially during long incubation times. Make sure the adhesive film is sealed around each well.

If your glycan-binding protein samples are fluorescently labelled, go directly to Part 6 – Final wash and dry.

Part 3 – Wash

1. Remove glycan-binding samples from each well by gently touching the pipette tip to the corner of the well of the cassette and tip the slide so that the sample pools to that corner. Avoid touching the array surface.
2. Add wash buffer to each well. We recommend using 100 μL per well for 16 subarray cassettes and 200 μL for 8 subarray cassettes. Cover the wells with adhesive film and incubate on the shaker for 5 minutes at 85 rpm. Completely remove the wash buffer by pipette and repeat this step. Avoid allowing the slide to dry out and have your next wash or sample ready before you remove the wash buffer.

If your glycan-binding sample is biotinylated, go directly to Part 5 – Fluorescent staining.

Part 4 – Binding of biotinylated antibody (Sandwich Assay Format)

1. Unless the secondary biotinylated antibody sample is bacteria or cells, centrifuge samples briefly to avoid adding irrelevant particles to the array.
2. After completely removing the wash buffer immediately add of the secondary biotinylated antibody to each well. We recommend using 100 μL per well for 16 subarray cassettes and 200 μL for 8 subarray cassettes. Seal the wells with adhesive film and incubate on the shaker for 1 hour at 100 rpm. Shaking at faster speed may prevent protein aggregation. Longer incubation time is acceptable, but not necessary.
3. After incubation repeat Part 3 – Wash.

Part 5 – Fluorescent staining

1. Centrifuge fluorescent labeled streptavidin samples briefly to avoid adding irrelevant particles to the array.
2. After completely removing the wash buffer immediately add the fluorescently labelled streptavidin sample. 100 μL per well is recommended for 16 subarray cassettes and 200 μL for 8 subarray cassettes. Seal the wells with adhesive film and shield the wells from light with aluminum foil. Incubate on the shaker at 85 rpm for 1 hour. Longer incubation time is acceptable, but not necessary.

Part 6 – Final wash and dry

1. Touch the pipette tip to the corner of the well of the cassette and tip the slide so that the sample pools to that corner and remove it. Avoid touching the array surface.
2. Briefly rinse each well with wash buffer. 100 μL per well is recommended for 16 subarray cassettes and 200 μL for 8 subarray cassettes.
3. Completely remove the wash buffer by pipette. Avoid touching the array surface. Repeat steps 2 and 3.
4. Disassemble the cassette from the slide. For the provided cassette this can be done by holding the slide with one hand at the top and bottom edges and sliding out the cassette clips one by one with the other hand. If your provided cassette has metal clips, they can be removed by rotating the clip outwards from the bottom of the slide. When the clips have been removed, place the slide on the table and hold a small outer edge of the slide to the table as you gently peel the cassette off.
5. Immediately immerse the slide in a coplin jar or beaker full of wash buffer. Do not touch the surface of the array or allow the array surface to touch the sides of the beaker or jar.
6. Place the jar or beaker on the 60 rpm shaker for 10 minutes.
7. Decant the wash buffer from the jar or beaker while holding the slide in place (only touch the edge of the slide) and then add sterile de-ionized water to immerse the slide.
8. Place the jar or beaker on the 60 rpm shaker for 2 minutes.
9. Decant the water from the jar or beaker.
10. Allow the slide to dry completely in a clean, dust free environment before scanning.

Analysis

Scan the slide in a laser fluorescence scanner at the wavelength of emission for the fluorophore used. Adjust the laser power and PMT to obtain the highest possible signals without any being saturated. Analyze data with microarray analysis software. If there is specific binding the signal intensity should be significantly higher than the negative control signal. Our standard method of comparing signal intensities is to quantify the median signal intensity data and subtract the background intensity.

Interpretation of Control Signals:


Negative Control (Print Buffer): The negative control should produce little to no signal. Since there is no binding involved with the negative control, any other signals around the negative control's intensity are also not binding.

Marker: The array marker should show a fluorescence signal regardless of the assay. It is there primarily to aid with orientation of the array map during analysis.


Biotinylated Mannose (PC1): This positive control will bind directly to the fluorescent labelled streptavidin. If your glycan-binding protein sample is already fluorescently labelled, or in any case where the addition of fluorescent labelled streptavidin to the array was not performed (Part 5 – Fluorescent staining) this positive control will not be reactive.

IgG (PC2, PC3, PC4): IgG is an antibody found in blood that is a primary component of humoral immunity. If the glycan-binding or secondary antibody sample is an anti-IgG antibody from human, mouse, or rabbit it should bind to the respective IgG control.

Typical Binding Assay Result from the N-Glycan Array

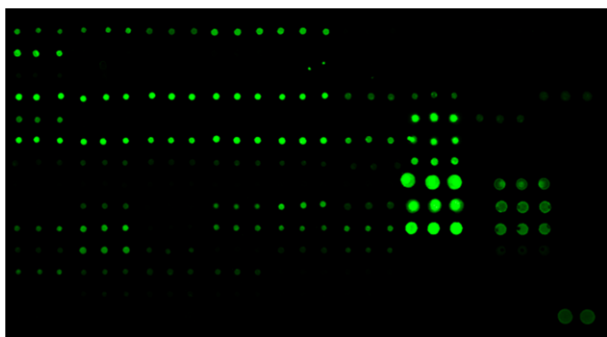

Example 1: N-glycan array on 8 subarrays. A subarray assayed with glycan-binding protein biotinylated ConA lectin, followed by streptavidin-Cy3 conjugate. Array was scanned with a GenePix scanner at 475 PMT and 100% laser power at 532nm wavelength. There is no non-specific binding for the negative control spots. Positive control 1 and the marker show binding as expected, as well as mannose-containing N-glycans.

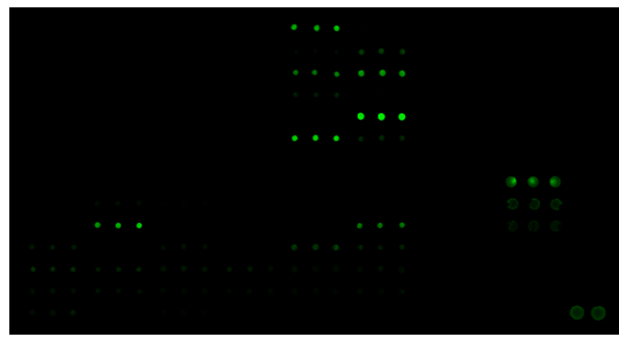

Example 2: N-glycan array on 8 subarrays. A subarray assayed with glycan-binding protein biotinylated AAL lectin, followed by streptavidin-Cy3 conjugate. Array was scanned with a GenePix scanner at 475 PMT and 100% laser power at 532nm wavelength. There is no non-specific binding for the negative control spots. Positive control 1 and the marker show binding as expected, as well as fucosylated N-glycans.

Troubleshooting

Condition	Possible Causes	Potential Solutions
High Background	<ul style="list-style-type: none"> • Concentration of glycan-binding protein samples is too high • Concentration of fluorescent samples is too high. • Arrays are not thoroughly washed • Slide drying out during assay • Excessive particles in the samples due to sample aggregation, dust, etc. 	<ul style="list-style-type: none"> • Use a lower concentration range of samples. Consider a wider range if you are unsure where the detection limit is. • Apply longer times for washing steps and use a higher shaking rate • Make sure wash buffer and sample is completely removed before the next step • Make sure adhesive film fully seals the wells to avoid evaporation • Centrifuge the samples prior to assay to avoid adding irrelevant particles • If you think that the protein is aggregating during incubation, try shaking at a higher speed
Signal Variation	<ul style="list-style-type: none"> • Slide drying out during assay. • Binding samples are not equally distributed in the wells • Glycan-binding protein aggregation during incubation • Bubbles during incubation 	<ul style="list-style-type: none"> • Make sure wells are sealed to prevent evaporation during incubation. • Apply a larger volume of sample to each well to ensure equal distribution • Use a higher shaking rate during incubation • Make sure samples are homogeneous, mixed thoroughly, and do not leave bubbles on the array surface
Unexpected Binding	<ul style="list-style-type: none"> • Cross contamination between wells or other sources. • Sample contamination 	<ul style="list-style-type: none"> • Make sure to use sterilized pipette tips and tubes used for sample application and preparation • Ensure cassette is pressed firmly to the slide so that there are no gaps to allow leaking between wells • Be careful not to cross contaminate samples when applying to the wells, even during wash steps